

F/*ex*SH**MYC/IGH TriCheck Probe**

REF Z-2293-50

Σ 5 (0.05 ml)

For the qualitative detection of human MYC rearrangements with and without participation of the human IGH locus by fluorescence *in situ* hybridization (FISH)



In vitro diagnostic medical device  
according to EU directive 98/79/EC

**1. Intended use**

The F/*ex*SH MYC/IGH TriCheck Probe (PL247) is intended to be used for the qualitative detection of human MYC rearrangements with and without participation of the human IGH locus in formalin-fixed, paraffin-embedded specimens such as lymphoma tissue by fluorescence *in situ* hybridization (FISH). The probe is intended to be used in combination with the F/*ex*SH-Tissue Implementation Kit (Prod. No. Z-2182-5/-20).

Interpretation of the results must be made within the context of the patient's clinical history with respect to further clinical and pathologic data of the patient by a qualified pathologist.

**2. Clinical relevance**

The MYC proto-oncogene (a.k.a. CMYC) encodes a transcription factor essential for cell growth and proliferation and is broadly implicated in tumorigenesis. Translocations involving the MYC gene are considered to be cytogenetic hallmarks for Burkitt lymphoma (BL) but are also found in other types of lymphomas. The most frequent translocation involving the MYC gene region t(8;14) (q24.21;q32.3) can be found in approx. 80% of the BL cases and juxtaposes the MYC gene next to IGH (immunoglobulin heavy locus). Further translocations affecting the MYC gene are t(8;22)(q24.21;q11.2) and t(2;8)(p11.2;q24.21), both of which involve one of the two immunoglobulin light chain loci. All three translocations bring the MYC gene under the control of a regulatory element from one of the immunoglobulin loci resulting in constitutive overexpression of MYC. Large B-cell lymphoma patients with MYC-IG have shorter overall survival compared with both MYC translocation with non-IG translocation partner gene as well as absence of MYC translocation. Thus, the detection of MYC translocation partner by FISH may prove a valuable diagnostic and prognostic tool.

**3. Test principle**

The fluorescence *in situ* hybridization (FISH) technique allows for the detection and visualization of specific nucleic acid sequences in cell preparations. Fluorescently-labeled DNA fragments, so called FISH probes, and their complementary target DNA strands in the preparations are co-denatured and subsequently allowed to anneal during hybridization. Afterwards, unspecific and unbound probe fragments are removed by stringency washing steps. After counterstaining the DNA with DAPI, hybridized probe fragments are visualized using a fluorescence microscope equipped with excitation and emission filters specific for the fluorochromes with which the FISH probe fragments have been directly labeled.

**4. Reagents provided**

The F/*ex*SH MYC/IGH TriCheck Probe is composed of:

- ZyGreen (excitation 503 nm/emission 528 nm) labeled polynucleotides (~10.0 ng/μl), which target sequences mapping in 8q24.21\* (chr8:130,373,051-130,930,673) distal to the MYC breakpoint region (see Fig. 1).
- ZyOrange (excitation 547 nm/emission 572 nm) labeled polynucleotides (~2.5 ng/μl), which target sequences mapping in 8q24.21\* (chr8:127,888,765-128,363,281) proximal to the MYC breakpoint region (see Fig. 1).
- ZyBlue (excitation 418 nm/emission 467 nm) labeled polynucleotides (~70 ng/μl), which target sequences mapping in 14q32.33\* (chr14:105,462,169-106,995,000) harboring the IGH locus (see Fig. 1).
- Formamide based hybridization buffer

\*according to Human Genome Assembly GRCh37/hg19

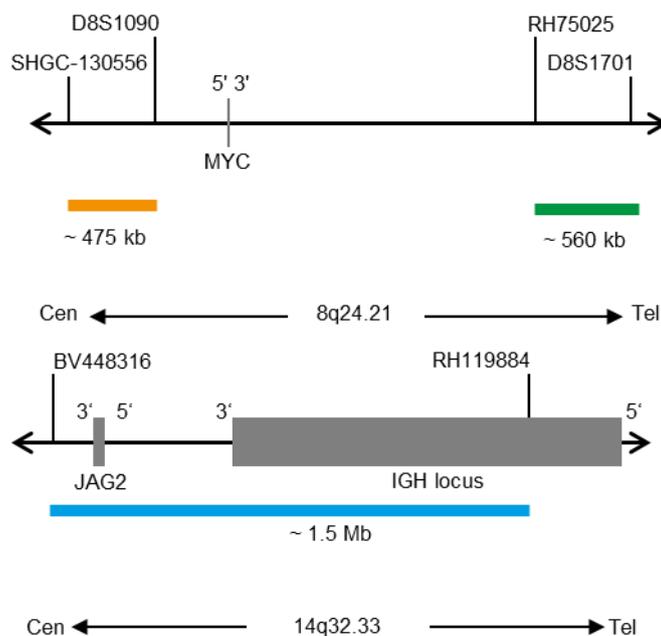


Fig. 1: Top: MYC Probe map; Bottom: IGH Probe map (not to scale)

The F/*ex*SH MYC/IGH TriCheck Probe is available in one size:

- Z-2293-50: 0.05 ml (5 reactions of 10 μl each)

**5. Materials required but not provided**

- F/*ex*SH-Tissue Implementation Kit (Prod. No. Z-2182-5/-20)
- Positive and negative control specimens
- Microscope slides, positively charged
- Water bath (37°C, 98°C)
- Hot plate or hybridizer
- Hybridizer or humidity chamber in hybridization oven
- Adjustable pipettes (10 μl, 25 μl)
- Staining jars or baths
- Timer
- Calibrated thermometer
- Ethanol or reagent alcohol
- Xylene
- Deionized or distilled water

- Coverslips (22 mm x 22 mm, 24 mm x 60 mm)
- Rubber cement, e.g., Fixogum Rubber Cement (Prod. No. E-4005-50/-125) or similar
- Adequately maintained fluorescence microscope (400-1000x)
- Immersion oil approved for fluorescence microscopy
- Appropriate filter sets

## 6. Storage and handling

Store at 2-8°C in an upright position protected from light.

Use protected from light. Return to storage conditions immediately after use. Do not use reagents beyond expiration date indicated on the label. The device is stable until expiration date indicated on the label when handled accordingly.

## 7. Warnings and precautions

- The probe should not be exposed to light, especially strong light, for a longer period of time, i.e. all steps should be accomplished, where possible, in the dark and/or using lightproof containers!
- Read the instruction for use prior to use!
- Do not use the reagents after the expiry date has been reached!
- This product contains substances (in low concentrations and volumes) that are harmful to health and potentially infectious. Avoid any direct contact with the reagents. Take appropriate protective measures (use disposable gloves, protective glasses, and lab garments)!
- If reagents come into contact with skin, rinse skin immediately with copious quantities of water!
- A material safety data sheet is available on request for the professional user.
- Do not reuse reagents.
- Avoid cross-contamination of samples as this may lead to erroneous results.

### Hazard and precautionary statements:

The hazard determining component is Formamide.



**Danger**

H319	Causes serious eye irritation.
H351	Suspected of causing cancer.
H360FD	May damage fertility. May damage the unborn child.
H373	May cause damage to organs through prolonged or repeated exposure.
P201	Obtain special instructions before use.
P260	Do not breathe dust/fume/gas/mist/vapours/spray.
P280	Wear protective gloves/protective clothing/eye protection/face protection.
P305+P351+P338	IF IN EYES: Rinse cautiously with water for several minutes. Remove contact lenses, if present and easy to do. Continue rinsing.
P308+P313	IF exposed or concerned: Get medical advice/attention.
P337+P313	IF eye irritation persists: Get medical advice/attention.

## 8. Limitations

- For *in vitro* diagnostic use.
- For professional use only.
- The clinical interpretation of any positive staining, or its absence, must be done within the context of clinical history, morphology, other histopathological criteria as well as other diagnostic tests. It is the responsibility of a qualified pathologist to be familiar with the FISH probes, reagents, diagnostic panels, and methods used to produce the stained preparation. Staining must be performed in a certified, licensed laboratory under the supervision of a pathologist who is responsible for reviewing the stained slides and assuring the adequacy of positive and negative controls.
- Specimen staining, especially signal intensity and background staining, is dependent on the handling and processing of the specimen prior to staining. Improper fixation, freezing, thawing, washing, drying, heating, sectioning, or contamination with other specimens or fluids may

produce artefacts or false results. Inconsistent results may result from variations in fixation and embedding methods, as well as from inherent irregularities within the specimen.

- The probe should be used only for detecting loci described in 4. "Reagents provided".
- The performance was validated using the procedures described in this instruction for use. Modifications to these procedures might alter the performance and have to be validated by the user.

## 9. Interfering substances

Red blood cells present in the specimen might exhibit autofluorescence which hinders signal recognition.

The following fixatives are incompatible with ISH:

- Bouin's fixative
- B5 fixative
- Acidic fixatives (e.g., picric acid)
- Zenker's fixative
- Alcohols (when used alone)
- Mercuric chloride
- Formaldehyde/zinc fixative
- Hollande's fixative
- Non-buffered formalin

## 10. Preparation of specimens

Prepare specimens as described in the instructions for use of the F/exlSH-Tissue Implementation Kit.

## 11. Preparatory treatment of the device

The product is ready-to-use. No reconstitution, mixing, or dilution is required. Bring probe to room temperature (18-25°C) before use, protect from light. Prior to opening the vial, mix by vortexing and spin down briefly.

## 12. Assay procedure

### Specimen pretreatment

Perform specimen pretreatment (dewaxing, proteolysis) according to the instructions for use of the F/exlSH-Tissue Implementation Kit.

### Denaturation and hybridization

1. Pipette 10 µl of the probe onto each pretreated specimen.
2. Cover specimens with a 22 mm x 22 mm coverslip (avoid trapped bubbles) and seal the coverslip.

*We recommend using rubber cement (e.g., Fixogum) for sealing.*

3. Place slides on a hot plate or hybridizer and denature specimens for 10 min at 75°C.
4. Perform hybridization for 2 h up to 16 h (i.e. overnight) at 37°C by either transferring the slides to a hybridizer or to a humidity chamber and a hybridization oven.

*It is essential that specimens do not dry out during the hybridization step.*

### Post-hybridization

Perform post-hybridization processing (washing, counter-staining, fluorescence microscopy) according to the instructions for use of the F/exlSH-Tissue Implementation Kit.

## 13. Interpretation of results

With the use of appropriate filter sets, the hybridization signals of the probe appear green (distal to the MYC breakpoint region), orange (proximal to the MYC breakpoint region), and blue (IGH locus).

**Normal situation:** In interphases of normal cells or cells without MYC rearrangements, two green/orange fusion signals appear when using an appropriate dual bandpass filter set and two blue signals appear when using an appropriate single bandpass filter set. When using an appropriate triple color bandpass filter set, two green/orange fusion signals and two blue signals can be observed (see Fig. 2).

**Aberrant situation:** A rearrangement of the MYC gene region not involving the IGH locus is indicated by a green/orange fusion signal, separated single green and orange signals and two blue signals. A MYC rearrangement involving the IGH locus is indicated by one green/orange fusion signal, one separate blue signal and one green/blue fusion signal as well as one orange/blue fusion signal. In a cell with a rearrangement of the IGH locus not involving the MYC gene or a trisomy of chromosome 14, two green/orange fusion signals and three blue signals can be observed (see Fig. 2).

*Overlapping green and orange signals may appear as yellow signals.*

	Green/Orange Dual Bandpass Filter Set	Blue Single Bandpass Filter Set	Merged Picture or Triple Bandpass Filter Set
Normal cells			
MYC rearrangement not involving IGH			
MYC rearrangement involving IGH			
IGH rearrangement not involving MYC or trisomy 14			

**Fig. 2: Expected results in normal and rearranged interphase nuclei**

Genomic aberrations due to small deletions, duplications or inversions might result in inconspicuous signal patterns.

Other aberrant signal patterns may be caused by complete or partial loss of IGHC or IGHV genes as well as cryptic insertions into other loci. Furthermore, absent or diminished blue signals on one or both alleles might represent deletions of IGHV genes resulting from normal somatic V-D-J recombination. Due to IGH homologous sequences in 16p11.2 and 15q11.2, faint cross-hybridizations may be observed. Other signal distribution may be observed in some abnormal samples which might result in different signal patterns than described above, indicating variant rearrangements. Unexpected signal patterns should be further investigated.

**Please note:**

- Due to decondensed chromatin, single FISH signals can appear as small signal clusters. Thus, two or three signals of the same size, separated by a distance  $\leq 1$  signal diameter, should be counted as one signal.
- Do not evaluate overlapping nuclei.
- Do not count over-digested nuclei (recognized by dark areas visible inside of the nuclei).
- Do not count nuclei with strong auto-fluorescence, which hinders signal recognition.
- A negative or unspecific result can be caused by multiple factors (see chapter 17).
- In order to correctly interpret the results, the user must validate this product prior to use in diagnostic procedures according to national and/or international guidelines.

**14. Recommended quality control procedures**

In order to monitor correct performance of processed specimens and test reagents, each assay should be accompanied by internal and external controls. If internal and/or external controls fail to demonstrate appropriate staining, results with patient specimens must be considered invalid.

**Internal control:** Non-neoplastic cells within the specimen that exhibit normal signal pattern, e.g., fibroblasts.

**External control:** Validated positive and negative control specimens.

**15. Performance characteristics**

**Accuracy:** The location of hybridization of the probe was evaluated on metaphase spreads of a karyotypically normal male. In all tested specimens the probe hybridized solely to the expected loci. No additional signals or cross-hybridizations were observed. Therefore, the accuracy was calculated to be 100%.

**Analytical sensitivity:** For the analytical sensitivity assessment, the probe was evaluated on metaphase spreads of karyotypically normal males. All nuclei showed the expected normal signal pattern in all tested specimens. Therefore, the analytical sensitivity was calculated to be 100%.

**Analytical specificity:** For the analytical specificity assessment, the probe was evaluated on metaphase spreads of karyotypically normal males. In all tested specimens, all signals hybridized solely to the expected target loci and no other loci. Therefore, the analytical specificity was calculated to be 100%.

**16. Disposal**

The disposal of reagents must be carried out in accordance with local regulations.

**17. Troubleshooting**

Any deviation from the operating instructions can lead to inferior staining results or to no staining at all.

**Weak signals or no signals at all**

Possible cause	Action
No target sequences available	Use appropriate controls
Specimen has not been properly fixed	Optimize fixing time and fixative
Heat pretreatment, proteolysis, denaturation, hybridization, or stringency wash temperature not correct	Check temperature of all technical devices used, using a calibrated thermometer
Proteolytic pretreatment not carried out properly	Optimize pepsin incubation time, increase or decrease if necessary
Probe evaporation	When using a hybridizer, the use of the wet stripes/water filled tanks is mandatory. When using a hybridization oven, the use of a humidity chamber is required. In addition, the coverslip should be sealed completely, e.g., with Fixogum, to prevent drying-out of the sample during hybridization.
Too low concentrated stringency wash buffer	Check concentration of stringency wash buffer
Old dehydration solutions	Prepare fresh dehydration solutions
Fluorescence microscope wrongly adjusted	Adjust correctly
Inappropriate filter sets used	Use filter sets appropriate for the fluochromes of the probe. <i>Triple-bandpass filter sets provide less light compared to single or dual-bandpass filter sets. Consequently, the signals may appear fainter using these triple-bandpass filter sets.</i>
Photo-damage of the probes/fluorophores	Accomplish hybridization and washing steps in the dark

**Cross hybridization signals; noisy background**

Possible cause	Action
Incomplete dewaxing	Use fresh solutions; check duration of dewaxing
Proteolytic pretreatment too strong	Optimize pepsin incubation time
Probe volume per area too high	Reduce probe volume per section/area, distribute probe dropwise to avoid local concentration

Slides cooled to room temperature before hybridization	Transfer the slides quickly to 37°C
Too high concentrated stringency wash buffer	Check concentration of stringency wash buffer
Washing temperature following hybridization too low	Check temperature; increase if necessary
Dehydration of sections between the individual incubation steps	Prevent dehydration by sealing the slides and performing incubation in humid environment

**Overlapping nuclei**

Possible cause	Action
Inappropriate thickness of specimen sections	Prepare 2-4 µm microtome sections

**Tissue morphology degraded**

Possible cause	Action
Specimen has not been properly fixed	Optimize fixing time and fixative
Proteolytic pretreatment not carried out properly	Optimize pepsin incubation time
Insufficient drying before probe application	Extend air-drying

**Specimen floats off the slide**

Possible cause	Action
Unsuitable slide coating	Use appropriate (positively charged) slides
Proteolytic pretreatment too strong	Shorten pepsin incubation time

**Weak counterstain**

Possible cause	Action
Low concentrated DAPI solution	Use <u>DAPI/DuraTect-Solution (ultra)</u> (Prod. No. MT-0008-0.8) instead
DAPI incubation time too short	Adjust DAPI incubation time

**18. Literature**

- Kievits T, et al. (1990) *Cytogenet Cell Genet* 53: 134-6.
- May P, et al. (2010) *Cancer Genet Cytogenet* 198: 71-5.
- Pedersen MØ, et al. (2014) *Eur J Haematol* 92: 42-8.
- Perkins AS & Friedberg JW (2008) *Hematology Am Soc Hematol Educ Program*: 341-8.
- Veronese ML, et al. (1995) *Blood* 85: 2132-8.
- Wilkinson DG: *In Situ Hybridization, A Practical Approach*, Oxford University Press (1992) ISBN 0 19 963327 4.

Our experts are available to answer your questions.  
Please contact [helptech@zytovision.com](mailto:helptech@zytovision.com)



ZytoVision GmbH  
Fischkai 1  
27572 Bremerhaven/ Germany  
Phone: +49 471 4832-300  
Fax: +49 471 4832-509  
[www.zytovision.com](http://www.zytovision.com)  
Email: [info@zytovision.com](mailto:info@zytovision.com)

**Trademarks:**  
ZytoVision® and F/exISH® are trademarks of ZytoVision GmbH.